


Glass pre-filled emergency syringe administration

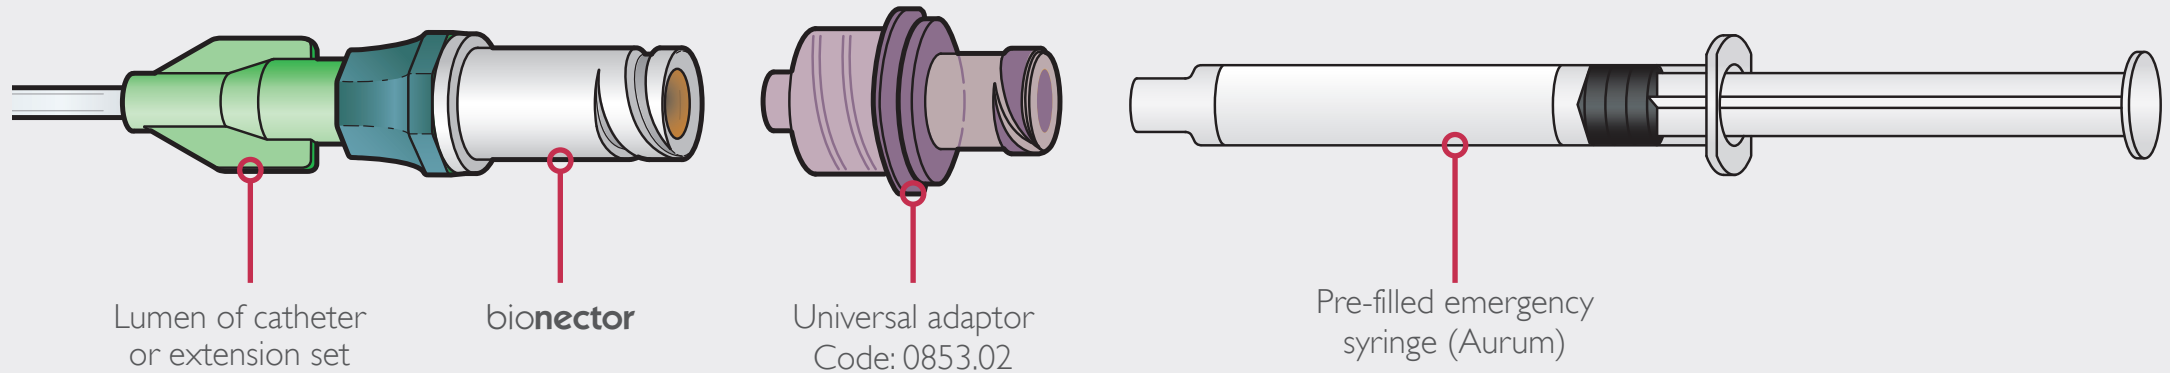

1. Attach the universal adaptor to the **bionector**
 2. Insert pre-filled glass emergency syringe (Aurum) into end of adaptor; then bolus as normal
 - 3. Remove the adaptor following administration of emergency drug(s).**
- If an adaptor is unavailable, remove the Bionector/extension set and access the cannula directly.